


Alcotest 7110 Calibration Record

Equipment


Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARXA-0056
Location:	LONG BRANCH POLICE DEPT		
Calibration File No.:	00629	Calib. Date:	10/21/2016
Certification File No.:	00594	Cert. Date:	04/22/2016
Linearity File No.:	00595	Lin. Date:	04/22/2016
Solution File No.:	00628	Soln. Date:	10/09/2016
Sequential File No.:	00629	File Date:	10/21/2016
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDXN S3-0217
Solution Control Lot:	16220	Expires:	09/07/2018
		Bottle No.:	0348

Coordinator

Last Name:	KLIMIK	First Name:	DAVID	MI:	W
Signature:				Badge No.:	7040
			#7040	Date:	10/21/2016

*Black Key Temperature Probe Serial.....# DDU5P2-003 (DK)

*Digital NIST Temperature Measuring System Serial.....# 150649679 (DK)

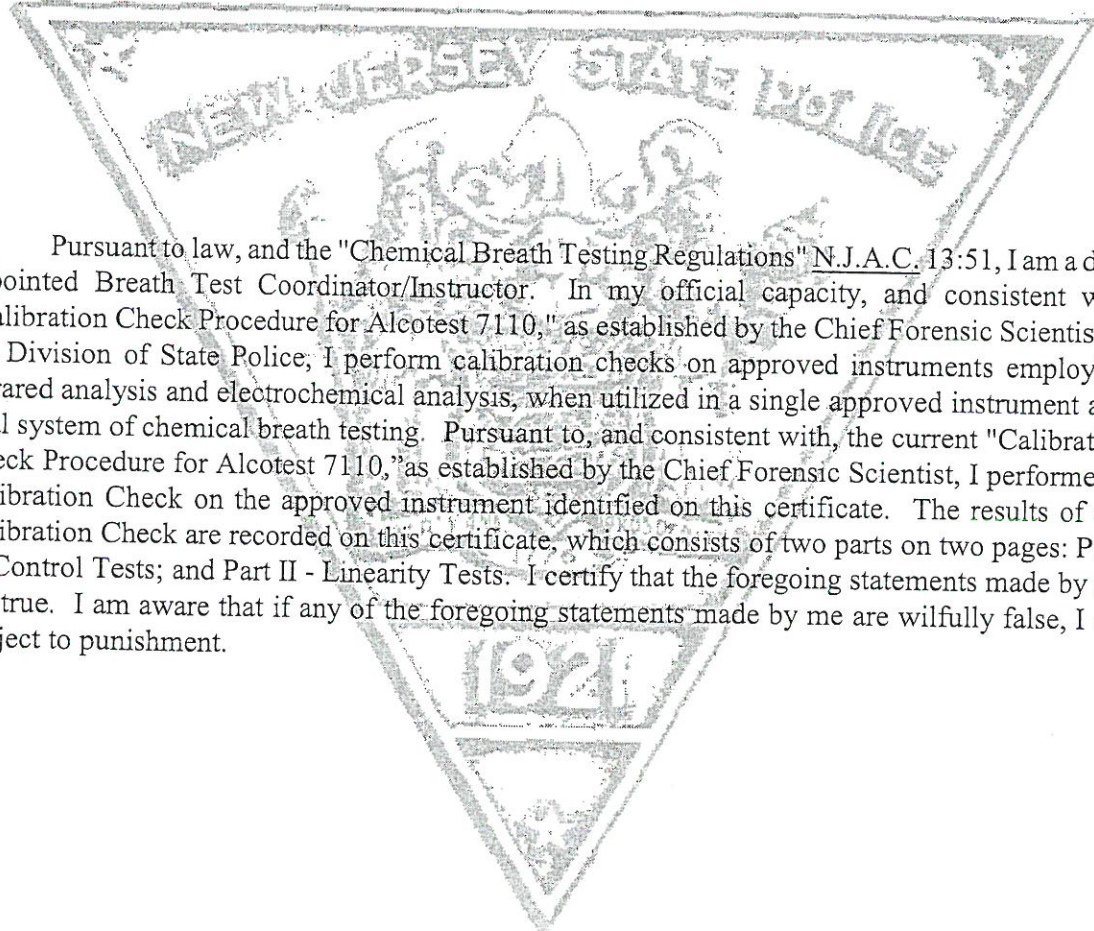

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part I - Control Tests

Equipment

Alcotest 7110 MKIII-C
Location: LONG BRANCH POLICE DEPT
Serial No.: ARXA-0056
Calibration File No.: 00629
Calib. Date: 10/21/2016
Calib. No.: 00025
Certification File No.: 00630
Cert. Date: 10/21/2016
Cert. No.: 00019
Linearity File No.: 00595
Lin. Date: 04/22/2016
Lin. No.: 00018
Solution File No.: 00628
Soln. Date: 10/09/2016
Soln. No.: 00126
Sequential File No.: 00630
File Date: 10/21/2016

Calibrating Unit: WET
Control Solution %: 0.100%
Solution Control Lot: 16220
Model No.: CU-34
Serial No.: DDXN S3-0217
Expires: 09/07/2018
Bottle No.: 0348

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	08:44D		
Control 1 EC	0.100%	08:45D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	08:45D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:46D		
Control 2 EC	0.099%	08:46D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.101%	08:46D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:47D		
Control 3 EC	0.100%	08:48D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	08:48D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:49D		

All tests within acceptable tolerance.

Coordinator

Last Name: KLIMIK

First Name: DAVID

MI: W

Signature:

Badge No.: 7040

Date: 10/21/2016

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor in my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to and consistent with the current "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXA-0056
Location:	LONG BRANCH POLICE DEPT	
Calibration File No.:	00629	Calib. Date: 10/21/2016
Certification File No.:	00630	Cert. Date: 10/21/2016
Linearity File No.:	00631	Lin. Date: 10/21/2016
Solution File No.:	00628	Soln. Date: 10/09/2016
Sequential File No.:	00631	File Date: 10/21/2016

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDRK S3-0005
Control Solution %:	0.040%		Expires: 09/19/2018
Solution Control Lot:	16230		Bottle No.: 1488

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDRF S3-0009
Control Solution %:	0.080%		Expires: 09/27/2018
Solution Control Lot:	16250		Bottle No.: 0544

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDCN-0054
Control Solution %:	0.160%		Expires: 10/03/2018
Solution Control Lot:	16260		Bottle No.: 1452

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	08:56D		
Control 1 EC	0.040%	08:57D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.039%	08:57D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:58D		
Control 2 EC	0.040%	08:59D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.038%	08:59D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:01D		
Control 3 EC	0.080%	09:01D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.079%	09:01D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:03D		
Control 4 EC	0.080%	09:04D	33.9°C	*** TEST PASSED ***
Control 4 IR	0.080%	09:04D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:05D		
Control 5 EC	0.160%	09:06D	34.0°C	*** TEST PASSED ***
Control 5 IR	0.159%	09:06D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:07D		
Control 6 EC	0.158%	09:08D	34.0°C	*** TEST PASSED ***
Control 6 IR	0.158%	09:08D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:09D		

All tests within acceptable tolerance.

Coordinator

Last Name: KLIMIK

First Name: DAVID

MI: W

Signature: TPR # 7. KLIMIK 7040

Badge No.: 7040

Date: 10/21/2016