

Alcotest 7110 Calibration Record

Equipment

Alcotest 7110 MKIII-C	Serial No.: ARXA-0056
Location: LONG BRANCH POLICE DEPT	
Calibration File No.: 00593	Calib. Date: 04/22/2016
Certification File No.: 00546	Calib. No.: 00024
Linearity File No.: 00547	Cert. Date: 10/16/2015
Solution File No.: 00592	Cert. No.: 00017
Sequential File No.: 00593	Lin. Date: 10/16/2015
	Lin. No.: 00017
	Soln. Date: 04/15/2016
	Soln. No.: 00119
	File Date: 04/22/2016


Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDXN S3-0216
Control Solution %: 0.100%		Expires: 08/17/2017
Solution Control Lot: 15H143		Bottle No.: 0648

Coordinator

Last Name: KLIMIK	First Name: DAVID	MI: W
Signature: <u>Tpa II D. Kl</u>	Badge No.: 7040	
	Date: 04/22/2016	

*Black Key Temperature Probe Serial.....# DDWAP2-024 (OK)

*Digital NIST Temperature Measuring System Serial.....# 150649679 (OK)

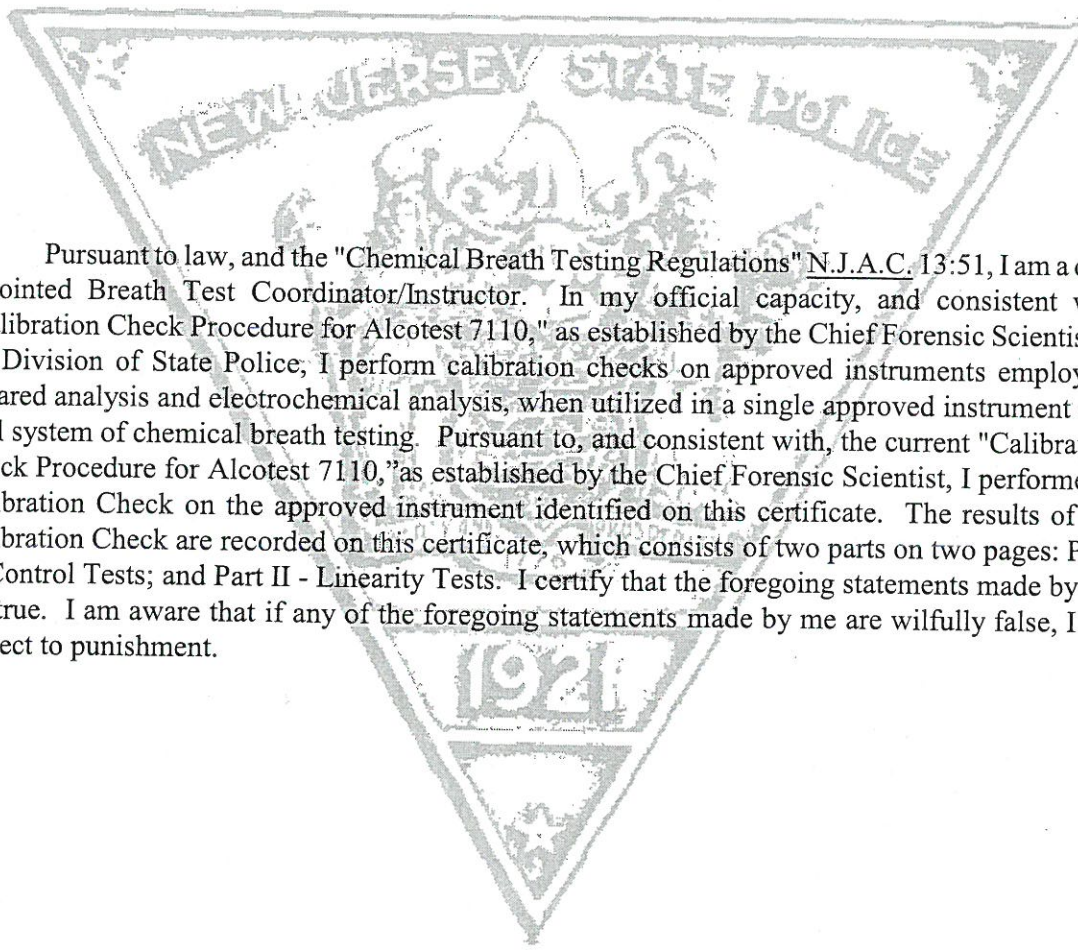

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part I - Control Tests

Equipment

Alcotest 7110 MKIII-C
Location: LONG BRANCH POLICE DEPT
Serial No.: ARXA-0056
Calibration File No.: 00593
Calib. Date: 04/22/2016
Calib. No.: 00024
Certification File No.: 00594
Cert. Date: 04/22/2016
Cert. No.: 00018
Linearity File No.: 00547
Lin. Date: 10/16/2015
Lin. No.: 00017
Solution File No.: 00592
Soln. Date: 04/15/2016
Soln. No.: 00119
Sequential File No.: 00594
File Date: 04/22/2016
Calibrating Unit: WET
Model No.: CU-34
Serial No.: DDXN S3-0216
Control Solution %: 0.100%
Expires: 08/17/2017
Solution Control Lot: 15H143
Bottle No.: 0648

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:00D		
Control 1 EC	0.099%	09:01D	34.1°C	*** TEST PASSED ***
Control 1 IR	0.098%	09:01D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:01D		
Control 2 EC	0.099%	09:02D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.097%	09:02D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:02D		
Control 3 EC	0.098%	09:03D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	09:03D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:04D		

All tests within acceptable tolerance.

Coordinator

Last Name: KLIMIK

First Name: DAVID

MI: W

Signature: T.P. D. KLIMIK

Badge No.: 7040

Date: 04/22/2016

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0056
Location: LONG BRANCH POLICE DEPT
Calibration File No.: 00593 **Calib. Date:** 04/22/2016 **Calib. No.:** 00024
Certification File No.: 00594 **Cert. Date:** 04/22/2016 **Cert. No.:** 00018
Linearity File No.: 00595 **Lin. Date:** 04/22/2016 **Lin. No.:** 00018
Solution File No.: 00592 **Soln. Date:** 04/15/2016 **Soln. No.:** 00119
Sequential File No.: 00595 **File Date:** 04/22/2016

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDRK S3-0005
Control Solution %: 0.040% **Expires:** 08/11/2017
Solution Control Lot: 15H141 **Bottle No.:** 0244

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDRF S3-0009
Control Solution %: 0.080% **Expires:** 08/13/2017
Solution Control Lot: 15H142 **Bottle No.:** 0272

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDWF S3-0223
Control Solution %: 0.160% **Expires:** 08/19/2017
Solution Control Lot: 15H144 **Bottle No.:** 0315

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:17D		
Control 1 EC	0.039%	09:18D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.039%	09:18D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:19D		
Control 2 EC	0.039%	09:20D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.039%	09:20D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:21D		
Control 3 EC	0.078%	09:22D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.078%	09:22D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:23D		
Control 4 EC	0.078%	09:24D	34.0°C	*** TEST PASSED ***
Control 4 IR	0.081%	09:24D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:25D		
Control 5 EC	0.157%	09:26D	34.1°C	*** TEST PASSED ***
Control 5 IR	0.158%	09:26D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:27D		
Control 6 EC	0.157%	09:28D	34.1°C	*** TEST PASSED ***
Control 6 IR	0.158%	09:28D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:29D		

All tests within acceptable tolerance.

Coordinator

Last Name: KLIMIK

First Name: DAVID

MI: W

Signature: _____

Part II D. Klimik #7040

Badge No.: 7040

Date: 04/22/2016